

HP07T SERIES RENEWAL

RENEWAL CONTENTS


Timing Adjustment Mechanism was improved by changing position of needle seal, and needle form.
 (※ Needle Height is 3mm longer than conventional product.)

MODEL CODE

HP07T-8JA → HP07TR-8JA


「R」 will be added as renewal product.

STRUCTURE

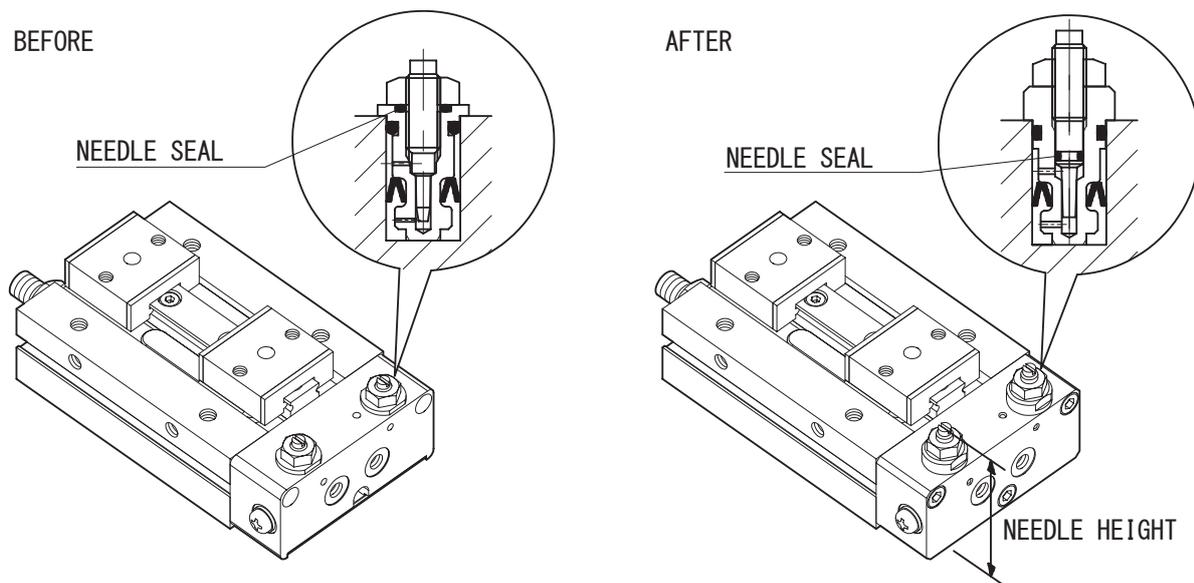

DIMENTION

<HP07TR-8>

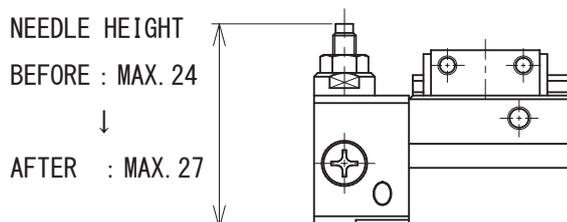

<HP07TR-12>

